


SEROLOGICAL PIPETTES



OPTIMIZED PIPETTING CONTROL

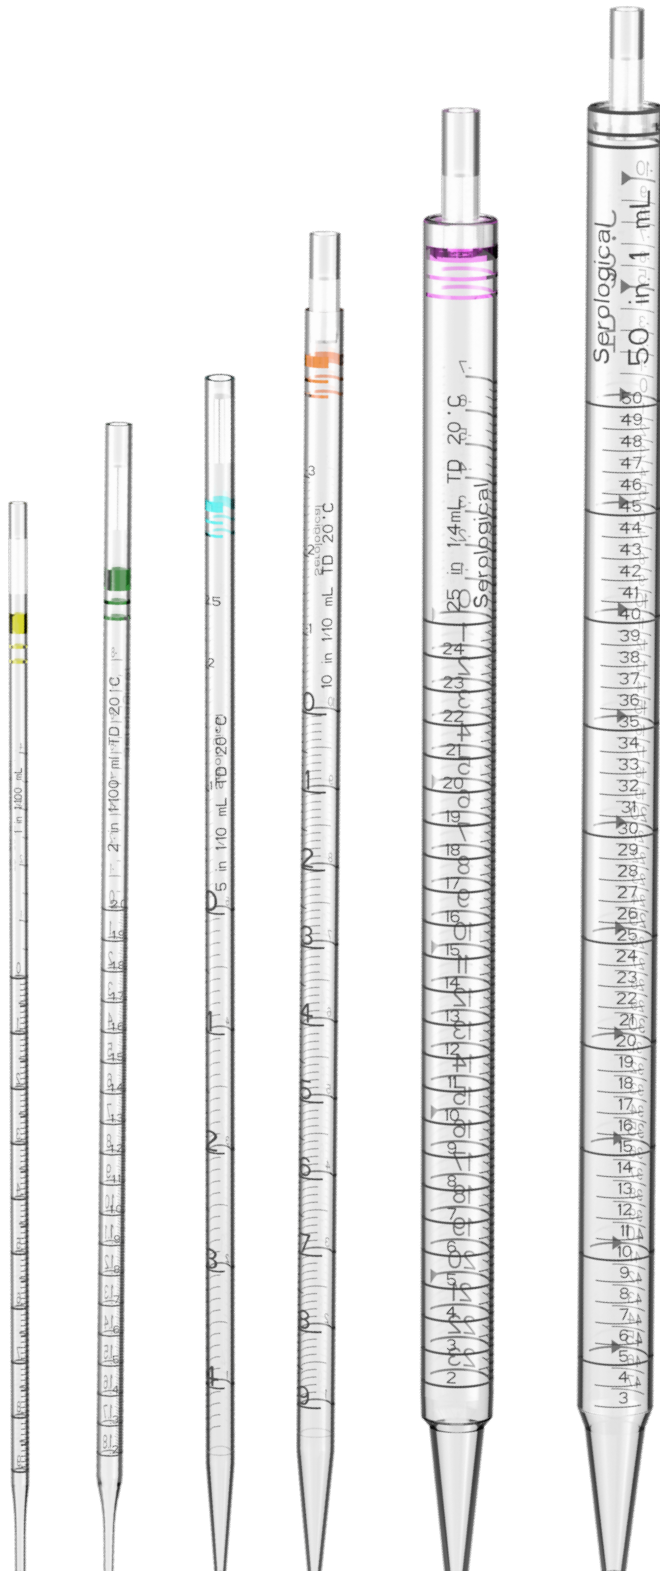

| Reliable

| Easy Volume Control

| Flexible



Reliable

Gilson serological pipettes are made with USP Class VI polystyrene and are free of contaminants that can alter your experiment. They are gamma-sterilized, non-pyrogenic, and certified free of detectable RNase/DNase. The polyester fiber plug provides a high level of protection against over-pipetting and contamination by liquids and aerosols.

Easy Volume Control

These serological pipettes contain color-coded rings for easy identification, as well as dark ascending and descending graduations so you can easily read the aspirated and dispensed volumes. They also have negative graduations for extra capacity.


Flexible

Available in models ranging from 1 to 50 mL, these serological pipettes are recommended for use with MACROMAN® and can also be used with any pipette controller. They enable precise and convenient dispensing of different kinds of liquids for a variety of tasks. The sterile, individually wrapped pipettes decrease the risk of contamination and are suitable for many applications.

Technical Information

SEROLOGICAL PIPETTES	
Accuracy	±3% (for 1 and 2 mL)
	±2% (for 5, 10, 25, and 50 mL)
Compliance	ISO 12771
Certifications	Non-pyrogenic
	RNase/DNase Free
	BSE/TSE Free
	Sterility: Gamma-irradiated
Materials	Pipette: USP Class VI polystyrene
	Plug: Polyester
Packaging	Bags of 25 or 20 sterile units
	Sterile, individually wrapped
Disposable	Yes

ORDERING INFORMATION			
MODEL	VOLUME	PART NUMBER	RING
Sterile bags of 25 units	1 mL	F110121	Yellow
	2 mL	F110123	Green
	5 mL	F110125	Blue
	10 mL	F110127	Red
Sterile bags of 20 units	25 mL	F110129	Purple
Sterile, individually wrapped	1 mL	F110122	Yellow
	2 mL	F110124	Green
	5 mL	F110126	Blue
	10 mL	F110128	Red
	25 mL	F110130	Purple
	50 mL	F110131	Black

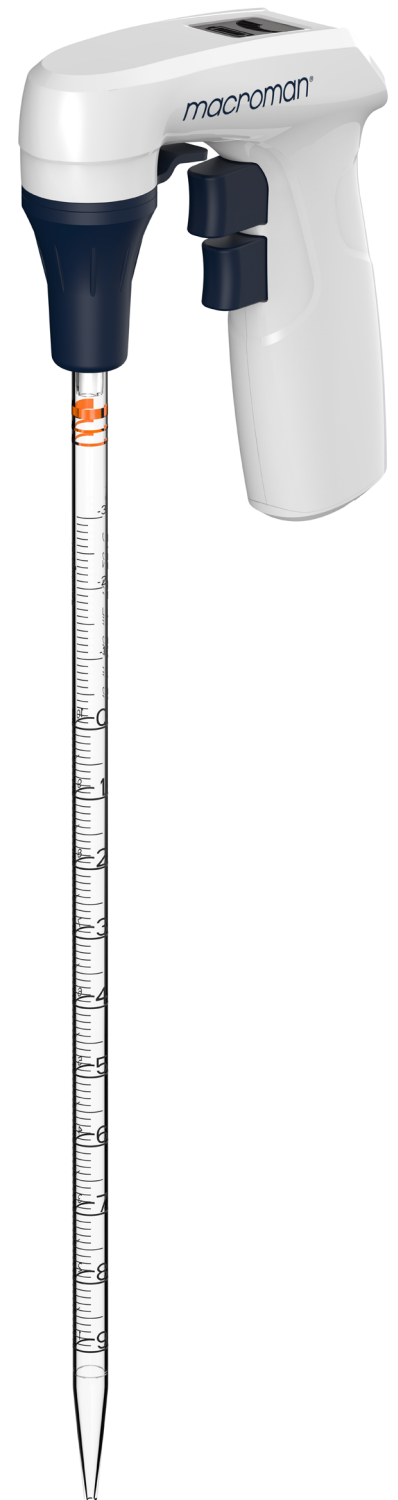

www.gilson.com/ContactUs

ISO 9001 LT800574/A | © 08/2018 Gilson S.A.S.
All rights reserved. All trademarks are the property of Gilson, Inc. and its subsidiaries.
CERTIFIED

